



**EKOTEKS LABORATUVAR ve GÖZETİM
HİZMETLERİ A.Ş.**
Esenyurt Firuzköy Bulvarı No:29 34325 Avcılar
İstanbul/ TÜRKİYE



TEST REPORT
DENEY RAPORU

AB-0583-T
20038356 -ing
10-20

Customer name:

ATS TÜKETİM MALLERİ SANAYİ VE TİC. A.Ş.

Address:

15 TEMMUZ MAHALLESİ 1498 SOKAK NO:24 JAT:1 GÜNEŞLİ
BAĞCILAR İSTANBUL

Buyer name:

-

Contact Person:

RIDVAN KARTAL

Order No:

-

Article No:

-

Name and identity of test item:

White non-woven mask. (Claimed to be; Colour Code: White)

The date of receipt of test item:

14.10.2020

**Re-submitted/re-confirmation
date:**

-

Date of test:

14.10.2020-23.10.2020

Remarks:

-

Sampling:

The results given in this report belong to the received sample by vendor.

End-Use:

-

Care Label:

Not Specified

Number of pages of the report:

5

The Turkish Accreditation Agency (TURKAK) is signatory to the multilateral agreements of the European co-operation for the Accreditation (EA) and of the International Laboratory Accreditation (ILAC) for the Mutual recognition of test reports. Deney laboratuvarı olarak faaliyeti gösteren EKOTEKS LABORATUVAR ve GÖZETİM HİZMETLERİ A.Ş. TÜRKAK'tan AB-0583-T akreditasyon dosya numarası ile ISO 17025:2017 standardına göre akredite edilmiştir.

The test and/or measurement results, the uncertainties (if applicable) with confidence probability and test methods are given on the following pages which are part of this report.



Date
26.10.2020

Customer Representative
Hatice ACARALP

Head of Testing Laboratory
Sevim A. RAZAK
26.10.2020

This report shall not be reproduced other than in full except with the permission of the laboratory.
Testing reports without signature and seal are not valid.

EKOTEKS LABORATUVAR ve GÖZETİM
HİZMETLERİ A.Ş.


AB-0583-T

20038356
-ing

10-20

REQUIRED TESTS	RESULT	COMMENTS
PHYSICAL PROPERTIES TESTS		
Breathability (Differential Pressure)	P	
Blood Splash Resistance	P	Type IIR
MICROBIOLOGICAL TEST		
Bacterial Filtration Efficiency (BFE)	P	
Microbial Cleanliness (Bioburden)	P	
P: Pass F: Fail R: Refer to retailer technologist.		
Test results were evaluated according to EN 14683:2019+AC:2019 limit values		

REMARK: Original samples are kept for 3 months and all technical records are kept for 5 years unless otherwise specified. If requested, measurement uncertainty will be reported. But unless otherwise specified, measurement uncertainty is not considered while stating compliance with specification or limit values. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. Tests marked (*) in this report are not included in the accreditation schedule.

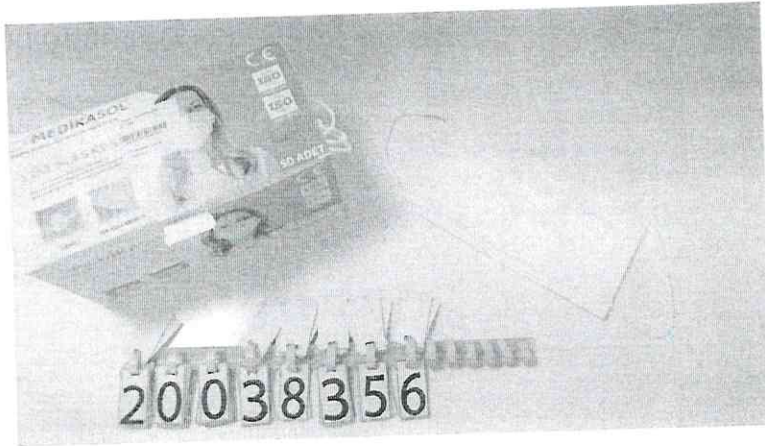

This report shall not be reproduced other than in full except with the permission of the laboratory.
Testing reports without signature and seal are not valid.

AB-0583-T

20038356
-ing

10-20

TEST RESULT

BREATHABILITY (Differential Pressure)

Test Metodu: EN 14683:2019+AC :2019 (TS EN 14683+AC:2019) EK-C

Test Condition (21 ± 5) °C ve (85 ± 5) % relative humidity, 4 hrs

Test area is 25 mm in diameter , 5 different sample was taken

Adjusted airflow is 8 l/min. The differential pressure is read directly using a differential pressure manometer .

SAMPLE	DIFFERENTIAL PRESSURE RESULT	REQUIREMENT
1	59.6 Pa/cm ²	< 60 Pa/cm ² Type I and Type II mask
2	55.3 Pa/cm ²	
3	44.4 Pa/cm ²	
4	43.7 Pa/cm ²	
Average Result	50.6 Pa/cm ²	

AB-0583-T

20038356
-ing

10-20

TEST RESULT

Medical face masks - Requirements and test methods EN 14683:2019+AC:2019 (TS EN 14683+AC:2019)

BACTERIAL FILTRATION EFFICIENCY (BFE)

Test Metodu: EN 14683:2019+AC :2019 (TS EN 14683+AC:2019) EK-B

A specimen of the mask material is clamped between a impactor and an aerosol chamber. An aerosol of *Staphylococcus aureus* is introduced into the aerosol chamber and drawn through the mask material and the impactor under vacuum. The bacterial filtration efficiency of the mask is given by the number of colony forming units passing through the medical face mask material expressed as a percentage of the number of colony forming units present in the challenge aerosol.

Test Flow Rate	28,3 L/min
Total Test Flow Time	2 minute
Sample Sizes	20x20 cm ²
Test Condition	(21 ± 5) °C and (85 ± 5) % relative humidity, 4 hours
Test Microorganism	<i>Staphylococcus aureus</i> ATCC 6538
Bacterial concentration (cfu/ ml)	5x10 ⁵ cfu/ ml
incubation conditions	24 hour, 35°C ± 2°C
Positive control sample average of number of Bacteria (C)	2.5x10 ³ cfu/ ml
Mean particle size (MPS)	3.0 µm

RESULTS			
Number of Test Sample	Test Sample (T) Number of Bacteria (cfu)	Bacterial Filtration Efficiency (% B)	Requirement BFE (%)
1	51	%98.1	Type I ≥95
2	44	%98.4	Type II ≥98
3	40	%98.5	
4	41	%98.5	
5	55	%98.0	

cfu: Colony-forming unit

$$B = (C - T) / C \times 100$$

%B: Bacterial Filtration Efficiency

C: is the mean of the total plate counts for the two positive control runs

T: is the total plate count for the test specimen

AB-0583-T

20038356
-ing

10-20

TEST RESULT

MICROBIAL CLEANLINESS (Bioburden)

Test Metod: EN 14683:2019+AC :2019 (TS EN 14683+AC:2019) EK-D
EN ISO 11737-1:2018 /TS EN ISO 11737-1 :2018

5 sample were taken. The sample is weighted and put in extraction liquid after shaking well (250 rpm, 5 min), inoculated on the suitable agar.

The plates are incubated for 3 days at 30 ± 1 °C for 72 hours, and 7 days at (20 to 25) °C for TSA and SDA plates respectively. Total microorganisms counts are calculated.

	RESULTS	REQUIREMENT
Microbial cleanliness (cfu/g)	19 kob/g	≤ 30 cfu/g Type I and Type II mask

*cfu= Colony forming unit.

BLOOD SPLASH RESİSTANCE

Test Metod: EN 14683:2019+AC :2019 (Clause 5.2.4) the resistance of the medical face mask to penetration

ISO 22609 :2004 Clothing for protection against infectious agents — Medical face masks — Test method for resistance against penetration by synthetic blood (fixed volume, horizontally projected)

Test Condition (21 ± 5) °C ve (85 ± 5) % relative humidity, 4 hrs
6 different sample was taken

	<u>SPLASH RESİSTANCE</u> <u>PRESSURE (kPa)</u>	<u>RESULTS</u>	<u>REQUIREMENT</u>
1	>21.3 kPa	PASS	≥ 16 kPa Type IIR mask
2	>21.3 kPa	PASS	
3	>21.3 kPa	PASS	
4	>21.3 kPa	PASS	
5	>21.3 kPa	PASS	
6	>21.3 kPa	PASS	
Average Result	>21.3 kPa	PASS	